


kab8-1

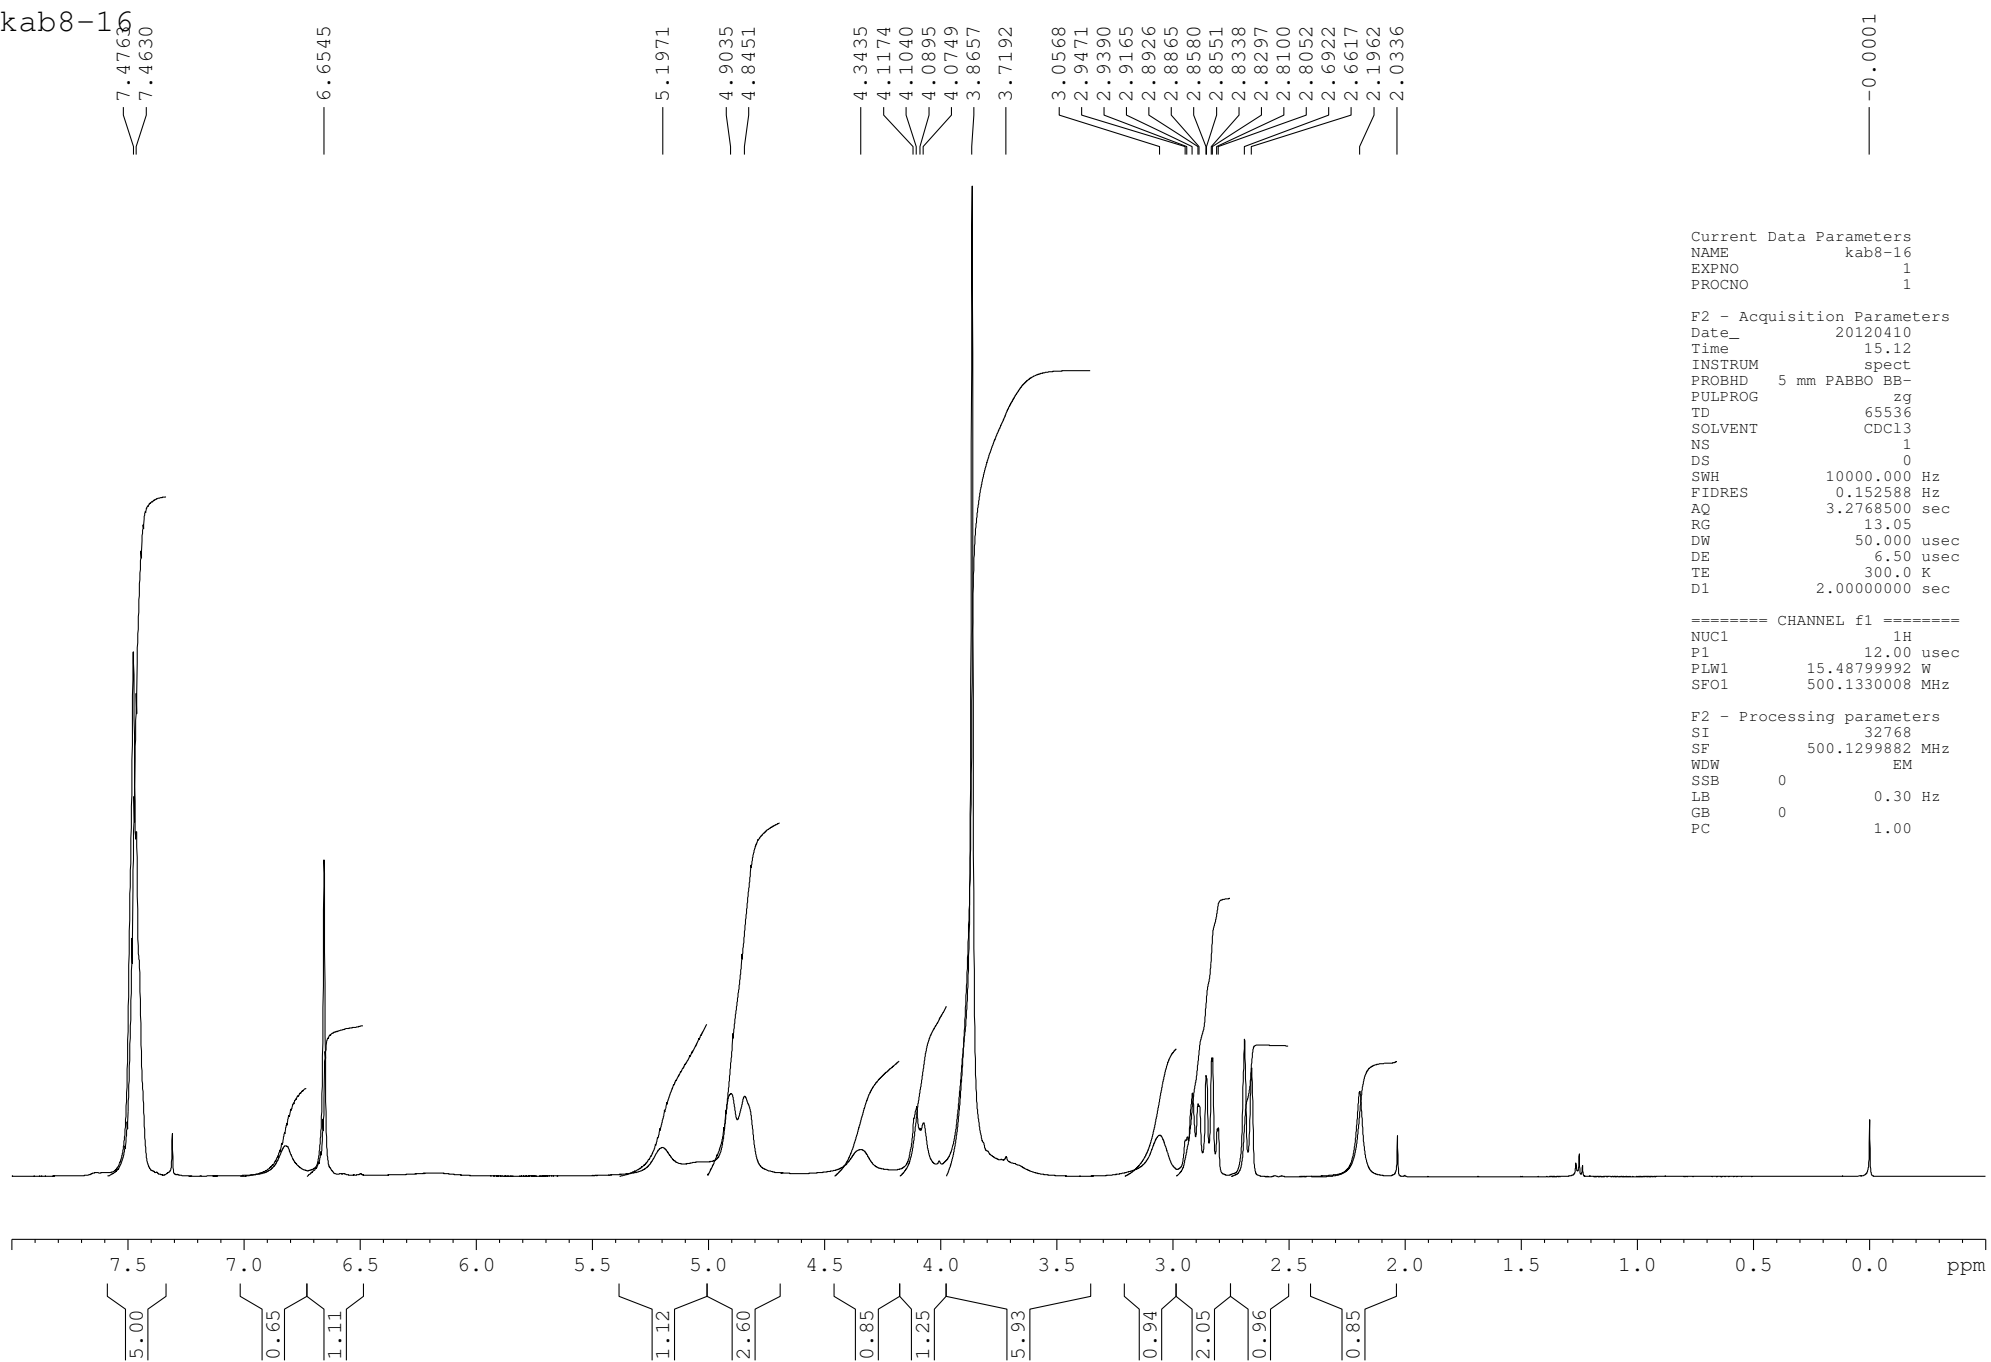

```
Current Data Parameters
NAME          kab8-16
EXPNO         1
PROCNO        1

F2 - Acquisition Parameters
Date_         20120410
Time_         15.12
INSTRUM       spect
PROBHD        5 mm PABBO BB-
PULPROG       zg
TD             65536
SOLVENT       CDCl3
NS             1
DS             0
SWH           10000.000 Hz
FIDRES        0.152588 Hz
AQ            3.2768500 sec
RG            13.05
DW            50.000 usec
DE            6.50 usec
TE            300.0 K
D1            2.00000000 sec

===== CHANNEL f1 =====
NUC1           1H
P1             12.00 usec
PLW1          15.48799992 W
SF01          500.1330008 MHz

F2 - Processing parameters
SI             32768
SF            500.1299882 MHz
WDW            EM
SSB            0
LB             0.30 Hz
GB            0
PC             1.00
```