


kab8-16

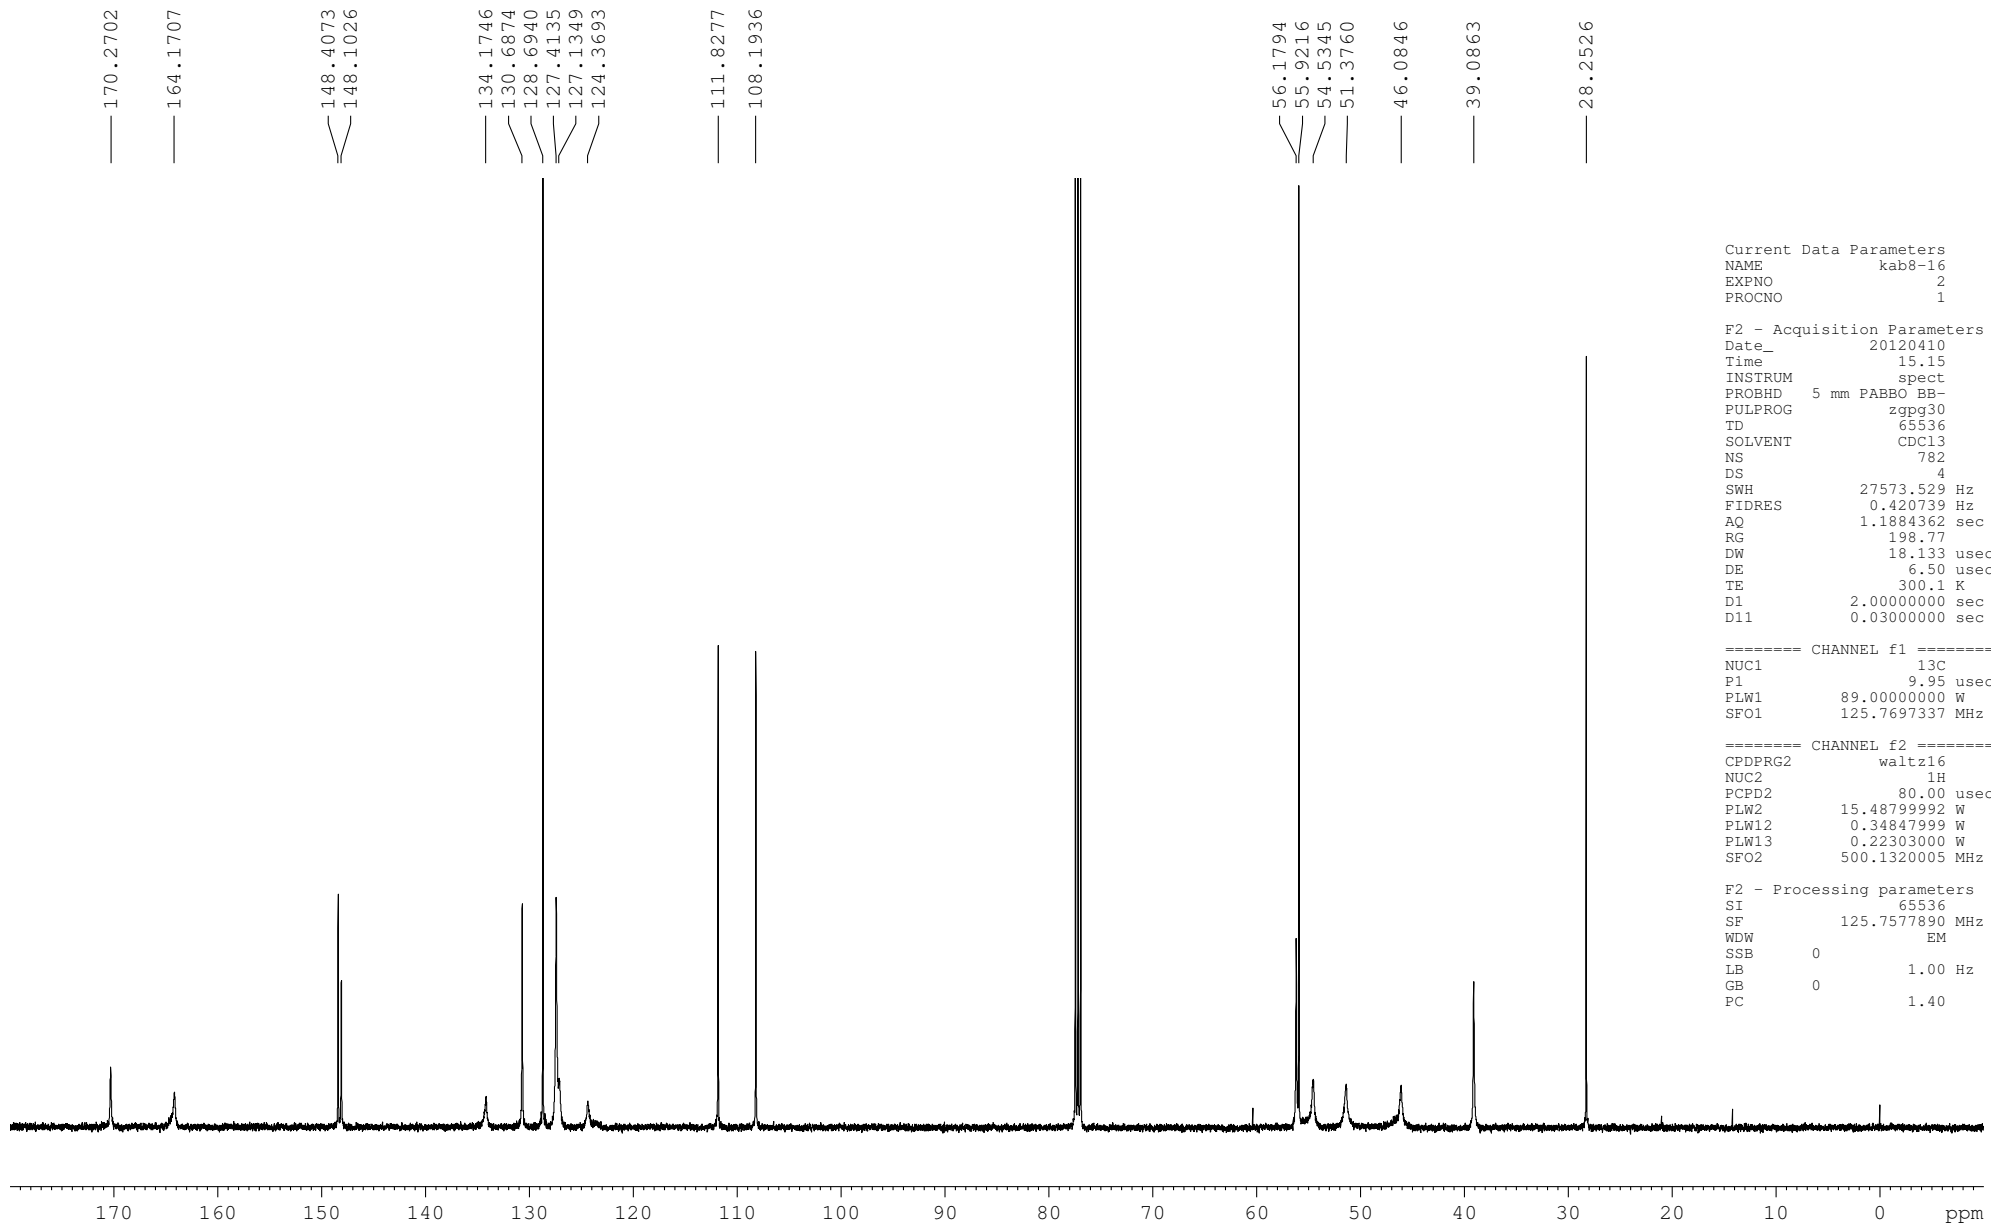

```
Current Data Parameters
NAME kab8-16
EXPNO 2
PROCNO 1

F2 - Acquisition Parameters
Date_ 20120410
Time 15.15
INSTRUM spect
PROBHD 5 mm PABBO BB-
PULPROG zgpg30
TD 65536
SOLVENT CDCl3
NS 782
DS 4
SWH 27573.529 Hz
FIDRES 0.420739 Hz
AQ 1.1884362 sec
RG 198.77
DW 18.133 usec
DE 6.50 usec
TE 300.1 K
D1 2.0000000 sec
D11 0.0300000 sec

===== CHANNEL f1 =====
NUC1 13C
P1 9.95 usec
PLW1 89.00000000 W
SFO1 125.7697337 MHz

===== CHANNEL f2 =====
CPDPRG2 waltz16
NUC2 1H
PCPD2 80.00 usec
PLW2 15.48799992 W
PLW12 0.34847999 W
PLW13 0.22303000 W
SFO2 500.1320005 MHz

F2 - Processing parameters
SI 65536
SF 125.7577890 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40
```